

**Center for Veterinary Biologics
and
National Veterinary Services Laboratories
Testing Protocol**

**Supplemental Assay Method for Detecting Lymphoid
Leukosis Biocontamination by the COFAL Test**

Date: June 26, 2000

Supersedes: July 1, 1973

Number: PYSAM0405.01

Standard Requirement: 9 CFR, Part 113.31

Contact Person: Rebecca L. W. Hyde (515)663-7336

Approvals:

Rebecca L. W. Hyde, Head
Poultry Biologics Virology Section

Date: _____

Ann L. Wieggers, Quality Assurance Manager

Date: _____

Randall L. Levings, Director
Center for Veterinary Biologics-Laboratory

Date: _____

United States Department of Agriculture
Animal and Plant Health Inspection Service
P. O. Box 844
Ames, IA 50010

Mention of trademark or proprietary product does not constitute a guarantee or warranty of the product by USDA and does not imply its approval to the exclusion of other products that may be suitable.

Supplemental Assay Method for Detecting Lymphoid Leukosis Biocontamination by
the COFAL Test

Table of Contents

1. Introduction
 - 1.1 Background
 - 1.2 Keywords
2. Preparation for the test
 - 2.1 Personnel qualifications/training
 - 2.2 Preparation of equipment/instrumentation
3. Part I. Propagation of extraneous lymphoid leukosis virus in Chick Embryo Fibroblasts (CEFs)
 - 3.1 Equipment/instrumentation
 - 3.2 Supplies
 - 3.3 Reagents
 - 3.4 Primary CEF preparation
 - 3.5 Secondary CEF preparation
 - 3.6 Preparation and inoculation of test material
 - 3.6.1 Avian encephalomyelitis (AE) vaccine (liquid glycerinated product)
 - 3.6.2 AE vaccine, lyophilized
 - 3.6.3 Hemorrhagic enteritis virus and marble spleen disease vaccine
 - 3.6.4 Infectious bronchitis vaccine, lyophilized or frozen
 - 3.6.5 Infectious bursal disease (IBD) vaccine, lyophilized or frozen
 - 3.6.6 Laryngotracheitis vaccine, lyophilized
 - 3.6.7 Marek's disease (MD) vaccine, cell associated, frozen
 - 3.6.8 MD vaccine, lyophilized
 - 3.6.9 Newcastle disease vaccine and combination Newcastle-bronchitis vaccine, lyophilized or frozen
 - 3.6.10 Pox and AE-pox combination vaccine
 - 3.6.11 Reovirus or tenosynovitis virus vaccine, lyophilized or frozen
 - 3.6.12 Recombinant virus vaccine

Supplemental Assay Method for Detecting Lymphoid Leukosis Biocontamination by
the COFAL Test

- 3.7 First and second harvest
- 3.8 Final harvest

4. Part II. Detection of extraneous lymphoid leukosis virus
group specific (gs) antigen by a microtiter Complement
Fixation (CF) test

- 4.1 Equipment/instrumentation
- 4.2 Reagents/supplies
- 4.3 Preparation and standardization of reagents
 - 4.3.1 Preparation of Veronal Buffered Diluent (VBD)
 - 4.3.2 Preparation and standardization of 2.8% sheep red blood suspension
 - 4.3.3 Preparation of hemoglobin color standards
 - 4.3.4 Hemolysin titration
 - 4.3.5 Preparation of sensitized cells
 - 4.3.6 Complement (C') titration
 - 4.3.7 Serum and antigen titrations

4.4 Detection of gs antigen in test material

5. Report of test results

6. Repeat tests

7. References

8. Summary of revisions

9. Appendix 1, Cell Counts

- 9.1 Materials
- 9.2 Counting cells with a hemacytometer
- 9.3 Formulating cell suspensions

**Supplemental Assay Method for Detecting Lymphoid Leukosis Biocontamination by
the COFAL Test**

1. Introduction

1.1 Background

This Supplemental Assay Method (SAM) describes a procedure for the detection of lymphoid leukosis virus biocontamination in live virus poultry vaccines. The Complement Fixation for Avian Leukosis (COFAL) test is a 2-part procedure: Part I. Propagation of lymphoid leukosis virus, if present, in Chick Embryo Fibroblast (CEF) cell culture, and Part II. Detection of the group-specific (gs) antigen by a microtiter complement-fixation technique.

NOTE: For this SAM, the dilution terminology of 1:10 specifies 1 part plus 9 parts (liquid).

1.2 Keywords

Avian lymphoid leukosis, COFAL, CF

2. Preparation for the test

2.1 Personnel qualifications/training

The personnel must have experience or training in this protocol. This includes knowledge of safe and aseptic biological laboratory techniques and preparation, proper handling, and disposal of biological agents, reagents, tissue culture samples, and chemicals. The personnel must also have training in the operation of the necessary laboratory equipment required for this assay.

2.2 Preparation of equipment/instrumentation

Operate and monitor all equipment/instrumentation according to manufacturers' instructions. Maintain aseptic conditions in a laminar flow biological safety cabinet, and use sterile instruments and wear sterile gloves when appropriate.

Supplemental Assay Method for Detecting Lymphoid Leukosis Biocontamination by
the COFAL Test

**3. Part I. Propagation of extraneous lymphoid leukosis virus in
CEFs**

3.1 Equipment/instrumentation

Equivalent equipment or instrumentation may be substituted
for any brand name listed below.

3.1.1 Laminar Flow Biological Safety Cabinet (NuAire
Inc., Labgard)

3.1.2 Humidified, rotating egg incubator (Midwest
Incubators, Model 252)

3.1.3 Water-jacketed incubator with a humidified
5% CO₂ atmosphere and temperature set at 37°C (Forma
Scientific, Model No. 3158)

3.1.4 Roller apparatus (to rotate roller bottles)

3.1.5 Centrifuge (Beckman J-6B, JS-4.2 rotor)

3.1.6 Vacuum pump (Curtin Matheson Scientific, Inc.)

3.1.7 Bunsen burner (Hanau Engineering Co.,
Touch-O-Matic)

3.1.8 Scissors, sterile (Roboz RS-6800)

3.1.9 Curved tip forceps, sterile (V. Mueller SU 2315)

3.1.10 Magnetic stir bars (sterile) and a stir plate

3.1.11 Hemacytometer (American Optical)

3.2 Supplies

Equivalent supplies may be substituted for any brand name
listed below. All supplies must be sterile.

3.2.1 Tissue culture dish, 150 x 10 mm (Falcon,
Cat. No. 1058)

**Supplemental Assay Method for Detecting Lymphoid Leukosis Biocontamination by
the COFAL Test**

- 3.2.2 Tissue culture dish, 100 x 20 mm (Falcon, Cat. No. 3003)
- 3.2.3 Plastic funnel covered with 4 layers of fine gauze
- 3.2.4 Conical tube, polypropylene, 29 x 114 mm, 50 ml (Sarstedt, Cat. No. 62.547.205)
- 3.2.5 Centrifuge tubes, Polypropylene, 250 ml (Corning, Cat. No. 25350)
- 3.2.6 Roller bottles, 2000 ml, 850 cm², with screw caps (Becton Dickinson, Cat. No. 3007)
- 3.2.7 Trypan Blue
- 3.2.8 Snap-cap tubes, 12 x 75 mm (Falcon, Cat. No. 2058)
- 3.2.9 Cell lifters (Costar, Cat. No. 3008)
- 3.2.10 Filtering flask, 1 L, with hose and cannula
- 3.2.11 Serological pipettes
- 3.2.12 Erlenmeyer flasks
- 3.2.13 Syringes and needles
- 3.2.14 Membrane filters, 0.22 µ (Millipore, Cat. No. SLGA0250S)
- 3.2.15 Membrane filters, 0.45 µ (Millipore, Cat. No. SLHA0250S)
- 3.2.16 Membrane filters, 5.0 µ (Millipore, Cat. No. SLAP02550)

Supplemental Assay Method for Detecting Lymphoid Leukosis Biocontamination by
the COFAL Test

3.3 Reagents

Equivalent reagents may be substituted. All reagents must be sterile.

3.3.1 Two dozen 9- to 11-day-old Specific-Pathogen-Free (SPF) chick embryos from a genetic line of chickens (C/O) which are susceptible to all lymphoid leukosis virus subgroups

3.3.2 Growth Medium:

Medium 199 with Earle's salts	1	L
Bacto tryptose phosphate broth	50	ml
NaHCO ₃	1.5	g
Penicillin (potassium G)	100,000	units
Streptomycin sulfate	100	mg
Fetal bovine serum (FBS)(inactivated)	30-55	ml
Fungizone (optional)	2	mg

Adjust pH to 7.3 with NaHCO₃ solution

NOTE: Better cell growth and maintenance may occur if L-glutamine (10 ml/1000 ml growth medium = 1% L-glutamine) is added within 3 days prior to use of the medium.

If growth medium is used to wash embryonic tissues prior to trypsinization, omit the FBS and L-glutamine.

3.3.3 Puck's Saline A:

NaCl	8.0	g
KCl	0.4	g
Glucose	1.0	g
Phenol Red (0.5% solution)	1.0	ml
q.s. with distilled or deionized water	1	L

Adjust pH to 7.2 with NaHCO₃ solution.

**Supplemental Assay Method for Detecting Lymphoid Leukosis Biocontamination by
the COFAL Test**

3.3.4 Ethylenediamine tetraacetate (EDTA) Stock Solution (1.0%), also referred to as versene:

Add 1.0 g ethylenedinitrilo tetraacetic acid disodium salt to 100 ml Puck's saline A.

3.3.5 Trypsin Solution (0.25%):

Add 2.5 g trypsin to 1 L Puck's Saline A.
Add 0.35 g NaHCO_3 per L.
Adjust pH to 7.4 with NaHCO_3 solution.

Note: For trypsinizing embryos, use 0.25% trypsin solution as is.

For trypsinizing primary cultures, add 2.0 ml of 1% EDTA to 100 ml 0.25% trypsin solution, or 0.25% trypsin may be used as is.

For trypsinizing secondary or higher passage chick embryo cell cultures, mix 0.25% trypsin 1:5 (1 part trypsin plus 4 parts Puck's saline A) in Puck's saline A. Then add 2.0 ml of 1.0% EDTA solution per 100 ml trypsin solution. This makes a solution containing 0.05% trypsin and 0.02% EDTA. Add a few drops NaHCO_3 solution to bring the pH up to 7.2-7.4.

3.3.6 70% ethanol

3.4 Primary Chick Embryo Fibroblast (CEF) preparation

Primary CEF cultures can be prepared from 9- to 11-day-old genetically susceptible (C/O) embryos from a COFAL-negative chicken flock in the following manner, or alternate methods of preparation are acceptable:

3.4.1 Disinfect the air cell end of the egg with 70% ethanol, flame, and break open the shell with sterile forceps. Use the forceps to open the membranes, lift out the embryo, and place it in a sterile disposable 150 x 10-mm tissue culture or petri dish. Four to 24 embryos may be prepared together.

**Supplemental Assay Method for Detecting Lymphoid Leukosis Biocontamination by
the COFAL Test**

Remove (and discard) the heads and viscera of the embryos with sterile scissors and forceps. Wash the embryos several times with a 0.25% trypsin solution (room temp), a physiological saline solution, or growth medium without FBS or L-glutamine. Place the washed embryos in a sterile dry 150 x 10-mm tissue culture or petri dish and mince them thoroughly using sharp sterile scissors.

3.4.2 To further wash, put the minced tissue into a trypsinizing flask containing 50 ml growth medium without FBS or L glutamine, and a magnetic stir bar. Place the flask on a stir plate and stir with a moderate vortex for 5 min. Allow the cells to settle and decant (and discard) the supernatant and repeat.

3.4.3 To trypsinize the tissues, first rinse the residual media from the cells by adding 25 ml of the 0.25% trypsin solution, and then immediately decant the trypsin solution. Next add 50 ml of the 0.25% trypsin solution to the flask and mix on a magnetic stir plate for 20 min. (Set stir plate to produce a moderate vortex.)

3.4.4 Place a sterile gauze wrapped funnel into the opening of a 250-ml conical centrifuge tube. To stop the trypsinizing action on the cells, pour 2 ml of FBS through the gauze and then pour the trypsinized contents of the flask through the gauze funnel into the centrifuge tube. Bring the total volume to approximately 125 ml with growth media. Centrifuge for 10 min at 250 x g (1050 rpms using a Beckman J-6B centrifuge with a JS-4.2 rotor) with the temperature set at 10°C.

3.4.5 Observe and record the volume of packed cells, and then pour off the supernatant. Dilute the cells approximately 1:300 with growth medium. Plant 200 ml of diluted cell suspension in each 1000-ml roller bottle. Tighten the cap and incubate for 4 days in an incubator set at 37°C. (Alternately, if tissue culture flasks are planted, adjust the volume of cell

**Supplemental Assay Method for Detecting Lymphoid Leukosis Biocontamination by
the COFAL Test**

suspension appropriately, leave the caps loose, and incubate in a humidified incubator with the temperature set at 37°C and the atmosphere set at 5% CO₂ for 4 days.) After 4 days, the cell sheet should be well proliferated and ready to split.

3.5 Secondary CEF preparation

Secondary CEF cultures can be prepared in the following manner, or alternate methods of preparation are acceptable:

3.5.1 Decant the medium from 1 roller bottle of primary CEFs, pipetting any remaining media with a 5-ml pipette, and add 15 ml of the 0.25% trypsin solution prewarmed to 37°C. Rotate the bottle until the cells begin to detach, approximately 1 min. (The proper length of time will be learned by experience. Too short a time will result in large clumps of cells in the new suspension.) Decant the trypsin and, with an open hand, strike the side of the roller bottle until most of the cells become detached. Rinse the inside of the roller bottle with 15 ml of growth medium and swirl. Pipette the suspension with the cells into an empty Erlenmeyer flask. Repeat twice more for a total of 3 rinses. Repeat the above steps separately for each additional roller bottle.

3.5.2 Pour the combined cell suspension from the Erlenmeyer flask through a funnel covered with 4 layers of fine gauze into a second Erlenmeyer flask containing a sterile stir bar and 25 ml of growth medium for each roller bottle used. Then rinse the funnel with an additional 25 ml of medium for each roller bottle used. Thoroughly mix the cell suspension.

3.5.3 Make a cell count with a hemocytometer. (A total cell count using crystal violet stain is satisfactory.) See **Appendix 1**. Adjust the volume so that the cell concentration is approximately 500,000 cells per ml.

**Supplemental Assay Method for Detecting Lymphoid Leukosis Biocontamination by
the COFAL Test**

3.5.4 Plant the secondary cell suspension into the vessels to be used for the test (usually 60-mm or 100-mm plastic tissue culture dishes). Use 5 ml of the suspension for a 60-mm dish and 15 ml of the suspension for a 100-mm dish. The cultures are now ready to be inoculated with test materials.

3.6 Preparation and inoculation of test material

This protocol is designed primarily to detect infective lymphoid leukosis virus contamination in live virus poultry vaccines. Preparation procedures described are those which are least complicated, but still have been found in most cases to be adequate for the purpose. A suggested procedure for each type of vaccine is described separately. If the test materials are to be diluted for inoculation, regular growth medium or medium without serum can be used. In each case, add the inoculum to the plates in addition to the growth medium already in the plates. The test material may be inoculated immediately after planting the cell cultures if experience has shown the material used will not be toxic to chick embryo fibroblasts. After inoculation, incubate the cultures in a humidified incubator set at 37°C and containing 5% CO₂. Sixteen to 24 hr later, remove the fluids and replace with fresh growth medium added at the original planting volume of 5 ml per 60-mm plate or 15 ml per 100-mm plate.

Note: With materials that may be somewhat toxic, allow the cell sheets to attach and grow for 18 hr prior to adding the test inoculum, and then leave inoculum on the cells for 4-24 hr depending on the toxic effect.

3.6.1 Avian encephalomyelitis (AE) vaccine (liquid glycerinated product)

This product tends to be somewhat toxic to the cell cultures, and the procedure for inoculation needs to be adjusted accordingly. Dilute the vaccine with tissue culture medium so that 1000 doses are present in

**Supplemental Assay Method for Detecting Lymphoid Leukosis Biocontamination by
the COFAL Test**

20 ml total volume. Centrifuge the mixture for 30 min at 1800 x *g* (3000 rpms using a Beckman J-6B centrifuge with a JS-4.2 rotor).

The solids will be primarily in the bottom, the fat-containing portion on top, and an aqueous portion in the middle. Insert a pipette into the aqueous portion and remove more than 10 ml. Filter this through a 5.0-micron membrane filter. Divide a quantity of filtrate equal to 500 doses (10 ml) among 5, 60-mm plates or 2, 100-mm plates. With this product, it is not known how much, if any, the vaccine virus or other vaccine components interfere with infection of the cells by leukosis virus.

3.6.2 AE vaccine, lyophilized

Restore this product with 1.0 ml tissue culture medium per 100 doses vaccine. If the product contains coarse tissue elements, centrifuge the restored material for 20 min at 1000 x *g* (2400 rpms using a Beckman J-6B centrifuge with a JS-4.2 rotor) and filter through a 0.45-micron membrane filter. Divide an amount of inoculum equal to 500 doses among 5, 60-mm plates or 2, 100-mm plates. To date, none of the products of this type have adversely affected the cell cultures. How much, if any, interference to infection of the cells by leukosis virus is caused by this vaccine virus is not known.

3.6.3 Hemorrhagic enteritis virus and marble spleen disease vaccine

Thaw or restore and dilute these products with 1.0 ml tissue culture medium per 100 doses vaccine. If the product contains coarse tissue elements, centrifuge the restored material for 20 min at 1000 x *g* (2400 rpms using a Beckman J-6B centrifuge with a JS-4.2 rotor) and filter through a 0.45 micron membrane filter. Divide an amount of inoculum equal to 500 doses among 5, 60-mm plates or 2, 100-mm plates. To date, none of the products of this type have adversely affected the

**Supplemental Assay Method for Detecting Lymphoid Leukosis Biocontamination by
the COFAL Test**

cell cultures. How much, if any, interference to infection of the cells by leukosis virus is caused by these vaccine viruses is not known.

3.6.4 Infectious bronchitis vaccine, lyophilized or frozen

Thaw or restore and dilute these products with 1.0 ml tissue culture medium per 100 doses vaccine. If the product contains coarse tissue elements, centrifuge the restored material for 20 min at 1000 x *g* (2400 rpms using a Beckman J-6B centrifuge with a JS-4.2 rotor) and filter through a 0.45-micron membrane filter. Divide an amount of inoculum equal to 500 doses among 5, 60-mm plates or 2, 100-mm plates. To date, none of the products of this type have adversely affected the cell cultures. How much, if any, interference to infection of the cells by leukosis virus is caused by this vaccine virus is not known.

3.6.5 Infectious bursal disease (IBD) vaccine, lyophilized or frozen

Thaw or restore and dilute this product with 1.0 ml tissue culture medium per 100 doses vaccine. Centrifuge the restored material for 20 min at 1000 x *g* (2400 rpms using a Beckman J-6B centrifuge with a JS-4.2 rotor) and filter through a 0.45-micron membrane filter. Neutralize the IBD virus with high titer specific antiserum (antiserum must be free of leukosis-sarcoma viruses and their antibodies). Mix 2 ml of the restored vaccine (200 doses) with 3 ml of the antiserum and incubate at room temperature for 1 hr. In some instances, a higher proportion of antiserum may be necessary. After the incubation period, inoculate the mixture, equivalent to 200 doses, into the cell cultures, dividing the entire amount equally among 5, 60-mm plates or 2, 100-mm plates.

**Supplemental Assay Method for Detecting Lymphoid Leukosis Biocontamination by
the COFAL Test**

3.6.6 Laryngotracheitis vaccine, lyophilized

Restore this product with 1.0 ml tissue culture medium per 100 doses vaccine. Centrifuge the restored material for 20 min at 1000 x g (2400 rpms using a Beckman J-6B centrifuge with a JS-4.2 rotor), and then filter through a 0.22-micron membrane filter. Divide an amount of inoculum equal to 500 doses among 5, 60-mm plates or 2, 100-mm plates.

**3.6.7 Marek's disease (MD) vaccine, cell associated,
frozen**

Thaw and dilute vaccine to 100 doses per 1.0 ml in tissue culture medium. Centrifuge 10.0 ml of the inoculum for 20 min at 1000 x g (2400 rpms using a Beckman J-6B centrifuge with a JS-4.2 rotor) and filter through a 0.22-micron membrane filter. Incubate at 25°-30°C for 20 to 30 min. Divide a quantity of filtrate equal to 500 doses among 5, 60-mm plates or 2, 100-mm plates.

3.6.8 MD vaccine, lyophilized

Restore this product with 1.0 ml tissue culture medium per 100 doses vaccine. Centrifuge the restored material for 20 min at 1000 x g (2400 rpms using a Beckman J-6B centrifuge with a JS-4.2 rotor) and filter through a 0.22-micron membrane filter. Neutralize 500 doses of the Marek's disease vaccine virus with high titer specific antiserum (antiserum must be free of leukosis-sarcoma viruses and their antibodies) and incubate at room temperature for 1 hr. After the incubation period, inoculate the mixture into the cell cultures, dividing the entire amount equally among 5, 60-mm plates or 2, 100-mm plates.

**Supplemental Assay Method for Detecting Lymphoid Leukosis Biocontamination by
the COFAL Test**

**3.6.9 Newcastle disease vaccine and combination
Newcastle-bronchitis vaccine, lyophilized or frozen**

Thaw or restore and dilute these products with 1.0 ml tissue culture medium per 100 doses vaccine. Neutralize the Newcastle disease virus (NDV) with high titer specific antiserum (antiserum must be free of leukosis-sarcoma viruses and their antibodies). Mix 2 ml of the restored vaccine (200 doses) with 2 ml of the NDV antiserum and incubate at room temperature for 1 hr. If the Newcastle vaccine is of particularly high titer, a higher proportion of antiserum may be necessary. After the incubation period, inoculate the mixture into the cell cultures, dividing the entire amount equally among 5, 60-mm plates or 2, 100-mm plates.

3.6.10 Pox and AE-pox combination vaccine

An optimum method for effectively neutralizing, inactivating, or separating out pox virus has not been determined, but the following method may be attempted. Thaw or restore and dilute these products with 10.0 ml tissue culture medium per 500 doses vaccine. Centrifuge for 20 min at 1000 x g (2400 rpms using a Beckman J-6B centrifuge with a JS-4.2 rotor) and filter through a 0.22-micron membrane filter. Divide an amount of inoculum equal to 500 doses among 5, 60-mm plates or 2, 100-mm plates.

**3.6.11 Reovirus or tenosynovitis virus vaccine,
lyophilized or frozen**

An optimum method for effectively neutralizing, inactivating, or separating out this virus has not been determined, but the following method may be attempted. Thaw or restore and dilute these products with 1.0 ml tissue culture medium per 100 doses vaccine. Centrifuge the restored material for 20 min at 1000 x g (2400 rpms using a Beckman J-6B centrifuge with a JS-4.2 rotor) and filter through a 0.45-micron membrane filter. Neutralize the reovirus or tenosynovitis virus

**Supplemental Assay Method for Detecting Lymphoid Leukosis Biocontamination by
the COFAL Test**

with high titer specific antiserum (antiserum must be free of leukosis-sarcoma viruses and their antibodies). Mix 2 ml of the restored vaccine (200 doses) with 2 ml of the antiserum and incubate at room temperature for 1 hr. In some instances, a higher proportion of antiserum may be necessary. After the incubation period, inoculate the mixture, equivalent to 200 doses, into the cell cultures, dividing the entire amount equally among 5, 60-mm plates or 2, 100-mm plates).

3.6.12 Recombinant virus vaccine

Follow the same method as for the vectoring agent.

Note: With each test series, maintain both positive and negative controls. Positive controls consist of 2 sets of plates, 1 inoculated with a subgroup A lymphoid leukosis virus, and 1 inoculated with a subgroup B lymphoid leukosis virus. Maintain a set of uninoculated plates as a negative control.

In all cases, remove the inoculum and medium in 24 hr or less after inoculating test material and add fresh growth medium.

Allow the cultures to grow for another 4 or 5 days without further treatment unless the pH of the medium becomes acid, necessitating a medium change.

At the end of this time, the first harvest of test material is made and the remaining cells are subcultured.

3.7 First and second harvest

3.7.1 Using an inverted microscope, examine each dish for contamination by bacteria or molds and to observe the condition of the cell sheet. Discard all contaminated plates and those with poor cellular growth. Harvest samples and passage cells as per **Sections 3.7.2-3.7.3**. Alternate methods are acceptable provided appropriate samples are harvested and cells

**Supplemental Assay Method for Detecting Lymphoid Leukosis Biocontamination by
the COFAL Test**

are split and transferred. It is not acceptable to seed the split cells onto a new cell sheet of CEFs.

Note: Process only 1 set of plates at a time and in the following order: negative controls, test samples, and then positive controls.

3.7.2 Tip the culture dishes slightly and, using a suction apparatus, remove all but approximately 0.25 ml of culture fluid from a 60-mm dish or 0.75 ml from a 100-mm dish. Use a sterile cell lifter and scrape off $\frac{1}{2}$ of the cell sheet from each plate into the remaining fluids. Remove and pool these cell suspensions for each set of test plates. Freeze these pools at -60°C or colder until the complement fixation (CF) test is conducted.

3.7.3 Subculture the remaining cells in the following manner: Add 0.05% trypsin (trypsin/Puck's saline, 1:5) plus 0.02% versene solution (3 ml per 60-mm dish, 5 ml per 100-mm dish) to each dish. Allow the trypsin solution to remain in contact with the cell sheet for 1-2 min, swirling occasionally, and then remove it immediately when the cells begin to detach from the plate. Let the dishes stand at room temperature until the cells loosen further. (Strike the plates sharply with the palm of the hand to facilitate cell detachment.) Add fresh growth medium to the dishes and disperse the cells with gentle pipetting. Pool these cell suspensions, mix thoroughly, and plant into new dishes. Plant 1 new culture dish for each original culture dish (a 2-for-1 split as $\frac{1}{2}$ the cells were saved for testing). Incubate these cultures at 37°C as before.

Note: The cultures will usually grow for 1 wk without a medium change, but if the pH becomes too acid, the medium will have to be changed in the interim. At the end of this wk period, handle the cultures exactly the same way as at the first subculture. Should the growth rate be so rapid that the cell sheet begins to peel

**Supplemental Assay Method for Detecting Lymphoid Leukosis Biocontamination by
the COFAL Test**

**before the scheduled time for subculture, an additional
harvest and subculture may be made.**

3.8 Final harvest

After this second subculture (postinoculation), maintain the cultures under the same conditions as before until the twenty-first day postinoculation, at which time a final harvest is conducted. At this final harvest, leave twice the fluid in each plate as before and scrape off the entire sheet with a cell lifter. Divide the final harvest (each test) and store a portion at -60°C or lower until after CF testing of the other portion is completed. If the CF testing of any particular series is inconclusive, the stored portion of the final harvest may be used as an inoculum for a new test series.

Cell culture fluids from each subculture or medium change are tested for extraneous lymphoid leukosis by the CF test.

**4. Part II: Detection of extraneous lymphoid leukosis virus
group specific (gs) antigen by a microtiter CF test**

The CF test method described has been adapted from the Laboratory Branch Complement Fixation (LBCF) Method developed at the National Communicable Disease Center, Atlanta, Georgia. The LBCF method is described in detail in Public Health Monograph No. 74. A supplement to this is entitled, "A Guide to the Performance of the Standardized Diagnostic Complement Fixation Method and Adaptation to Micro Test." First edition, July 1, 1969, has been prepared by the same Laboratory Section. These documents may be available from the Public Health Inquiries Branch, U.S. Public Health Service, Washington, D.C. 20201.

4.1 Equipment/instrumentation

Equivalent equipment or instrumentation may be substituted for any brand name listed below.

**Supplemental Assay Method for Detecting Lymphoid Leukosis Biocontamination by
the COFAL Test**

- 4.1.1 Centrifuge (Beckman J-6B, JS-3.0 rotor)
- 4.1.2 Incubator CO₂ (Forma Scientific, Model No. 3158)
- 4.1.3 Freezer, -70°C (Revco Scientific, Model No. ULT1790-7-ABA)
- 4.1.4 Water bath, 37°C ± 1°C
- 4.1.5 Mini-Orbital shaker (Bellco Glass, Cat. No. 7744-S0010)
- 4.1.6 Vortex mixer (Thermolyne Maxi Mix II, Model No. M37615)
- 4.1.7 Reading mirror (Cooke Engineering Co. Microtiter)
- 4.1.8 12-channel pipette (Labsystems Model Finnpipette Digital Multichannel 50-300 µl)
- 4.1.9 Pipettes (Labsystems Model Finnpipette Digital 5-40 µl & 40-200 µl)
- 4.1.10 Plate cover roller

4.2 Reagents/supplies

Equivalent reagents or supplies may be substituted for any brand name listed below.

- 4.2.1 Guinea pig complement (Whittaker Bioproducts, Cat. No. 30-956J)
- 4.2.2 Anti-sheep hemolysin and diluent (Baltimore Biological Laboratory)
- 4.2.3 Sheep blood (25 ml Alsevers + 25 ml sheep blood) 4-31 days after collection
- 4.2.4 Distilled or deionized water

**Supplemental Assay Method for Detecting Lymphoid Leukosis Biocontamination by
the COFAL Test**

4.2.5 Graduated Kolmer centrifuge tube, 10 ml (Corning Cat. No. 8360 or Kimble Cat. No. 45180)

4.2.6 Graduated cylinder, 100 ml

4.2.7 Erlenmeyer flasks, 125 & 250 ml

4.2.8 Beaker, 50 ml

4.2.10 Tissue culture 96-well U-shaped plate (Linbro, Cat. No. 76-013-05)

4.2.11 Adhesive plate cover (Dynatech Laboratories, Cat. No. 001-010-3501)

4.2.12 Polypropylene conical tube, 50 ml, 29 x 114 ml, sterile, (Sarstedt, Cat. No. 62.547.205)

4.2.13 Disposable polystyrene centrifuge tubes, 15 ml, 17 x 100-ml tubes (Falcon, Cat. No. 2057)

4.2.14 Disposable borosilicate serologic tubes, 3 ml, 12 x 75 mm

4.2.15 Snap cap tubes, 3 ml, 12 x 75 mm

4.2.16 Disposable serological pipettes, 1, 5, 10 and 25 ml

4.2.17 Pipette tips

4.2.18 Log-log paper

4.2.19 Plain graph paper

4.3 Preparation and standardization of reagents

4.3.1 Preparation of Veronal Buffered Diluent (VBD)

4.3.1.1 Preparation of the stock buffer solution
(5X VBD)

**Supplemental Assay Method for Detecting Lymphoid Leukosis Biocontamination by
the COFAL Test**

1. Combine the following in a 2-L volumetric flask in the order listed:

NaCl	83.00 g
Na-5, 5-diethyl barbiturate	10.19 g
Distilled water	1500 ml
1 N hydrochloric acid	34.58 ml
Stock solution containing 1.0 molar $MgCl_2$ and 0.3 molar $CaCl_2$ (20.3 g $MgCl_2 \cdot 6H_2O$ and 4.4 g $CaCl_2 \cdot 2H_2O$ in 100 ml distilled water)	5.00 ml

2. Fill to the 2-L mark with distilled water. Mix thoroughly.

3. Check the pH of the stock buffer before refrigeration by making a 1:5 dilution with distilled water (1 part 5X VBD plus 4 parts distilled water). The pH of the diluted stock (1X VBD) must be 7.3-7.4. If the pH is not in this range, discard and prepare fresh stock buffer.

4.3.1.2 Preparation of gelatin-water solution

1. Add 1.0 g of gelatin to 100 ml of distilled water. Bring to a boil to dissolve the gelatin.

2. Make up to 800 ml with sterile distilled water at room temperature.

3. Chill in the refrigerator. This solution should not be held longer than 1 wk.

**4.3.1.3 Preparation of VBD (1X) for daily use
(containing 0.1 percent gelatin)**

Add 4 volumes of gelatin water to 1 volume of 5X VBD stock buffer. Store in the refrigerator. VBD (1X) should not be stored longer than 24 hr.

Supplemental Assay Method for Detecting Lymphoid Leukosis Biocontamination by
the COFAL Test

NOTE: The pH of the VBD (1X) must be 7.3 to 7.4.

**4.3.2 Preparation and standardization of 2.8% sheep
red blood cell suspension**

4.3.2.1 Washing sheep cells (collected and
preserved in modified Alsever's solution; aged
4 days)

1. Add 2 or 3 volumes of cold VBD (1X) to each volume of preserved cells and centrifuge at 600 X g (1650 rpm in a Beckman J-6B centrifuge using a JS-3.0 rotor) for 5 min.
2. Carefully aspirate the supernatant fluid and the white cell layer without disturbing the erythrocytes.
3. Fill centrifuge tube again with cold VBD. Thoroughly resuspend the cells by gently mixing with a pipette. Centrifuge at 600 X g for 5 min and repeat the process for a total of 3 washings. If the supernate is not colorless after the second washing, the cells are too fragile and must not be used.
4. Resuspend the cells once more in cold VBD and centrifuge for 10 min at 600 X g to pack the cells.
5. Record the volume of packed cells in the centrifuge tube, and aspirate the supernate. Care should be taken to remove as much fluid as possible without disturbing the cells.

4.3.2.2 Standardization of 2.8% cell suspension

1. Prepare the 2.8% cell suspension (approximately 670,000 cells/mm³) by adding 34.7 vol of VBD to 1 vol of packed sheep

Supplemental Assay Method for Detecting Lymphoid Leukosis Biocontamination by
the COFAL Test

cells. (**Illustration 1**) Shake flask gently to insure even suspension of cells.

ILLUSTRATION 1

Standardization of Sheep Red Blood Cells to 2.8%

Cell Pack Volume (ml)	Adjust to Total Vol with VBD (ml)
0.5	17.9
0.6	21.4
0.7	25.0
0.8	28.6
0.9	32.1
1.0	35.7
1.1	39.3
1.2	42.8
1.3	46.4
1.4	50.0
1.5	53.6
1.6	57.1
1.7	60.7
1.8	64.3
1.9	67.8
2.0	71.4
2.1	75.0
2.2	78.5
2.3	82.1
2.4	85.7
2.5	89.3
2.6	92.8
2.7	96.4
2.8	100.0
2.9	103.5
3.0	107.1
3.1	110.7
3.2	114.2
3.3	117.8
3.4	121.4
3.5	125.0
3.6	128.5
3.7	132.1
3.8	135.6
3.9	139.2
4.0	142.8

**Supplemental Assay Method for Detecting Lymphoid Leukosis Biocontamination by
the COFAL Test**

2. To check the density of the 2.8% cell suspension, pipette 7.0 ml into a 10-ml graduated Kolmer centrifuge tube (either a Corning 8360 or Kimbal 45180 has acceptable tolerance) and centrifuge at 600 X g for 10 min. A 7.0 ml aliquot of properly prepared cell suspension should produce 0.2 ml of packed cells.

3. When the volume of packed cells is under or above the 0.2-ml point, the cell suspension should be adjusted. The quantity of VBD which must be added to or removed from the cell suspension is determined by the following formula, where PCV = actual packed cell volume of 7.0 ml

$$(PCV/0.20 \text{ ml}) \times 100 \text{ ml} = \text{corrected vol}$$

Example 1, low density: PCV = 0.19 ml

$$\frac{0.19 \text{ ml}}{0.20 \text{ ml}} \times 100 \text{ ml} = 95.0 \text{ ml}$$

Therefore, remove 5 ml of VBD from each 100 ml of cell suspension. (VBD may be removed by centrifuging an aliquot of the cell suspension and pipetting off the desired amount for discard.)

Example 2, high density: PCV = 0.21 ml

$$\frac{0.21 \text{ ml}}{0.20 \text{ ml}} \times 100 \text{ ml} = 105.0 \text{ ml}$$

Therefore, add 5.0 ml of VBD to each 100 ml of cell suspension.

Check the adjusted cell suspension by centrifuging a 7.0-ml portion as before.

Supplemental Assay Method for Detecting Lymphoid Leukosis Biocontamination by
the COFAL Test

NOTE: Keep the cell suspension in the refrigerator when not in use. Always swirl the flask gently before use to secure an even suspension of the erythrocytes.

4.3.3 Preparation of hemoglobin color standards

Eleven color standards are used to read the hemolysin, complement, and antigen titrations. These standards are prepared by combining proportionate amounts (**Illustration 2**) of hemoglobin solution and 0.28% cell suspension as follows:

4.3.3.1 Preparation of hemoglobin solution

1. Pipette 1.0 ml of the 2.8% cell suspension into a large test tube (17 x 100 mm).
2. Add 7.0 ml distilled water and shake the mixture until all cells are lysed.
3. Add 2.0 ml of the stock buffer solution (5X VBD) to restore tonicity and mix thoroughly.

4.3.3.2 Preparation of 0.28% cell suspension

Pipette 1.0 ml of the 2.8% cell suspension into a large test tube, add 9.0 ml of VBD, and mix thoroughly.

4.3.3.3 Preparation of color standards

1. Label 11 serologic tubes (12 x 75 mm) with the specified % of hemolysis shown in **Illustration 2**. Mix the varying ratios of hemoglobin solution and the 0.28% cell suspension as shown.

Supplemental Assay Method for Detecting Lymphoid Leukosis Biocontamination by
the COFAL Test

ILLUSTRATION 2

Reagents	Percent hemolysis									
	0	10	20	30	40	50	60	70	80	90
	100									
Hemoglobin	0	0.1	0.2	0.3	0.4	0.5	0.6	0.7	0.8	0.9
solution	1.0									
0.28 % cells	1.0	0.9	0.8	0.7	0.6	0.5	0.4	0.3	0.2	0.1
	0									

2. Shake the tubes and centrifuge at 600 X g for 5 min. Remove from the centrifuge without agitation. When not in use, store in refrigerator to prevent excessive change in color. The color standards, prepared for reading the complement titration, may be used the next day to read tests.

4.3.4 Hemolysin titration

4.3.4.1 Preparation of 1:100 hemolysin (rabbit antiserum against sheep red cells) solution

Thoroughly mix 98.0 ml of VBD and 2.0 ml of glycerinated hemolysin (lyophilized hemolysin with its glycerine containing diluent is equivalent). Dispense in convenient small aliquots and store at -20°C or lower. Do not refreeze after thawing.

4.3.4.2 Determination of hemolysin dilution needed for sensitization of 2.8% sheep cells

Perform a hemolysin titration each time a new lot of 1:100 hemolysin solution is prepared and each time a new lot of sheep cells is used.

1. Place 6 serologic tubes (12 x 75 mm) in a rack and label with hemolysin dilutions shown in last column of **Illustration 3**. Prepare dilutions for titration as shown. Thoroughly mix each dilution.

Supplemental Assay Method for Detecting Lymphoid Leukosis Biocontamination by
the COFAL Test

Note: These final hemolysin dilutions have been found appropriate for commercially prepared hemolysins. If they are not satisfactory, prepare other dilutions that suffice for the particular lot of hemolysin in routine use.

ILLUSTRATION 3

Preparation of Hemolysin Dilutions

Hemolysin dilution, 1 ml	Diluent, ml	Final hemolysin dilution
1:100-----plus	9.0-----gives	1:1000
1:1000-----plus	1.0-----gives	1:2000
1:1000-----plus	1.5-----gives	1:2500
1:1000-----plus	2.0-----gives	1:3000
1:1000-----plus	3.0-----gives	1:4000
1:1000-----plus	7.0-----gives	1:8000

2. Label a second set of 6 serologic tubes with the correct hemolysin dilutions. Add 1.0 ml of the standardized 2.8% sheep cell suspension to each tube.

3. Add 1.0 ml of each of the final hemolysin dilutions (1:1000 through 1:8000) to the 1.0-ml portions of sheep cell suspension with constant swirling of the contents. Incubate for 15 min at 37°C. After the incubation period, the sheep erythrocytes are "sensitized cells," ready for use.

4. Make a 1:400 dilution of guinea pig complement (C') by drawing up undiluted C' in a 1.0-ml pipette beyond the 0.6-ml mark. Wipe the tip of the pipette and return excess C' above the 0.6-ml mark to the stock container. Deliver 0.25 ml of C', without

**Supplemental Assay Method for Detecting Lymphoid Leukosis Biocontamination by
the COFAL Test**

using the last 0.1 ml of graduation of the pipette, into 99.75 ml of cold VBD. The diluted C' must be kept cold and be used within 2 hr.

NOTE: With less active C', it may be necessary to use a 1:300 dilution, or with a more potent C', a 1:500 dilution may be needed for proper results.

5. Label 6 serologic tubes with the final hemolysin dilutions. To each tube add 0.4 ml of cold VBD, 0.4 ml of the 1:400 C' dilution, and 0.2 ml of cells sensitized with the series of final hemolysin dilutions (step 3 above) to the properly labeled tube. Mix and incubate in a 37°C water bath for 30 min. Centrifuge at 600 X g to pack the cells. Read the % hemolysis in each tube by comparing with the color standards.

6. Plot the amount of hemolysis obtained with each dilution of hemolysin on ordinary graph paper. Determine the optimal dilution of hemolysin from the graph by inspection. It is desirable to select a dilution such that further increase in hemolysin (as the curve progresses to the right) does not appreciably change the % lysis. The dilution selected also needs to provide for a slight excess of hemolysin. See **Illustration 4**.


NOTE: On the X-axis, let the left end of the hemolysin dilution scale be 0, and measure a suitable length for the 1:1000 dilution. Other dilutions are represented as fractions of this length. Thus 1:2000 = 1/2 the length of 1:1000; 1:2500 = 2/5 of 1:1000; 1:3000 = 1/3 of 1:1000; 1:4000 = 1/4 of 1:1000; and 1:8000 = 1/8 of 1:1000.

Supplemental Assay Method for Detecting Lymphoid Leukosis Biocontamination by
the COFAL Test

ILLUSTRATION 4

Hemolysin titration

NOTE: Increasing the hemolysin concentration (left to right)

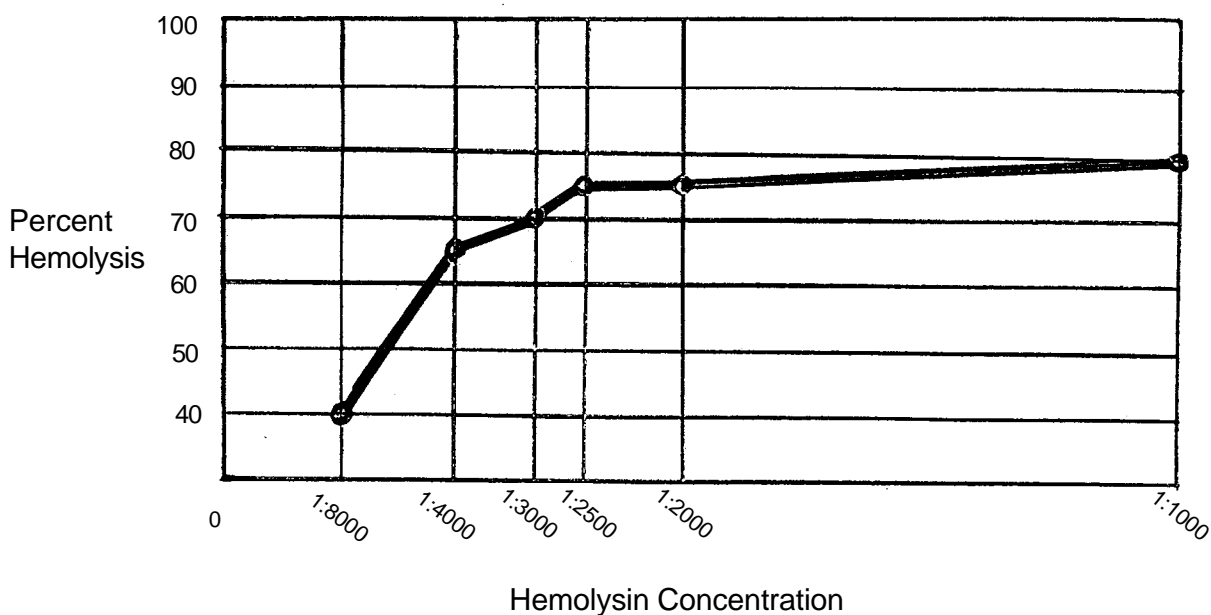

with the complement held constant results in a "plateau" from which the optimal hemolysin dilution is selected. The optimal hemolysin dilution in this instance is 1:2000.

4.3.5 Preparation of sensitized cells

1. Add 1 volume of optimal hemolysin dilution (example, 1:2000 dilution shown in **Illustration 4**) to 1 volume of the standardized 2.8% cell suspension with rapid, but gentle, swirling.
2. Before using, incubate for 15 min at 37°C.

Supplemental Assay Method for Detecting Lymphoid Leukosis Biocontamination by
the COFAL Test

4.3.6 Complement (C') titration

NOTE: For routine qualitative testing, the following procedure for handling complement has been found to be satisfactory: Commercially obtained lyophilized guinea pig complement is restored as directed. A 1:20 dilution of restored C' is made in 1X VBD; this dilution is dispensed in convenient (amount to be used at one time for tests) aliquots into inert plastic vials and stored at -70°C or colder. The C' dilution is thawed (10°C water bath) and further diluted for titration. After the titer is determined, the remaining vials are thawed and diluted as needed for test use. A vial of each batch so prepared should be titered every 2 wk to check for changes. There may be no significant decrease in titer over a period of several mo.

Titration of C' is performed as follows:

1. Prepare sensitized cells.
2. Label 4 serologic (12 x 75 mm) tubes as in **Illustration 5**. To obtain accuracy, titrate in duplicate and use the average hemolysis.
3. Prepare 1:400 dilution of C'. (The 1:400 dilution of C' prepared previously and stored in the refrigerator may be used for titrations of complement and hemolysin when performed at the same time.)
4. Add reagents in the order shown in **Illustration 5**.
5. Shake tubes and place in the 37°C water bath for 30 min. Shake once at 15 min.

Supplemental Assay Method for Detecting Lymphoid Leukosis Biocontamination by
the COFAL Test

ILLUSTRATION 5

Complement Titration

Reagent	Tube Number			
	1	2	3	4
VBD	0.6 ml	0.55 ml	0.5 ml	0.4 ml
1:400 dilution of C'	0.2 ml	0.25 ml	0.3 ml	0.4 ml
Sensitized cells	0.2 ml	0.2 ml	0.2 ml	0.2 ml

6. Remove tubes from water bath and centrifuge 600 X g to pack the cells. Determine the % hemolysis in each tube by comparing with the color standards, interpolating to the nearest 5% when a tube does not exactly match 1 of the standards.

ILLUSTRATION 6

Conversion of % lysed cells, y, to ratio of % lysed to non-lysed cells, $y/100-y$

y	$y/100-y$	y	$y/100-y$	y	$y/100-y$
10	0.111	40	0.67	70	2.33
15	0.176	45	0.82	75	3.00
20	0.25	50	1.0	80	4.0
25	0.33	55	1.22	85	5.7
30	0.43	60	1.50	90	9.0
35	0.54	65	1.86		

Supplemental Assay Method for Detecting Lymphoid Leukosis Biocontamination by the COFAL Test

7. Record the % hemolysis (y) for each tube. Using the chart in **Illustration 6**, determine the ratio of % lysed to non-lysed cells, $y/100-y$, for each vol (ml) of the 1:400 C', as shown in the example below. The "y" values are hypothetical.

Example:

<u>Tube #</u>	<u>Vol (ml) of</u> <u>1:400 C'</u>	<u>% Hemolysis</u> <u>(y)</u>	<u>Ratio</u> <u>(y/100-y)</u>
1	0.20	25	0.33
2	0.25	40	0.67
3	0.30	70	2.33
4	0.40	85	5.70

8. For each of the 4 tubes, plot on log-log graph paper the volume of the 1:400 dilution of C' in ml against the ratio found in the chart. (Do not graph when "y" exceeds 90% nor when "y" is less than 10%.) Join the 2 points plotted for the first 2 tubes and find the midpoint as shown in **Illustration 7**. Do the same for the last 2 tubes. (A good titration should have 2 points on each side of 1). Draw a line through the 2 midpoints. Draw a horizontal line through the intersection of this line with the vertical "I" line and read the C'H₅₀ in ml of the 1:400 dilution of C'. Five C'H_{50s} are required in the diagnostic test.

In the example, C'H₅₀ is 0.27 ml. Five units are contained in 1.35 ml (5 X 0.27) of the 1:400 dilution. The dilution of C' necessary to obtain 5 C'H_{50s} in 0.4 ml is calculated as follows:

$$\frac{400}{1.35} = \frac{x}{0.4} \quad 1.35 x = 160 \quad x = 118.5 \text{ or } 119$$

Supplemental Assay Method for Detecting Lymphoid Leukosis Biocontamination by
the COFAL Test

Hence 0.4 ml of a 1:119 dilution of C' contains 5 C'H_{50s}. (Direct readings for proper dilutions may be found in **Illustration 8.**)


Note: 0.4 ml of this working dilution of C' contains 5 units of C'H₅₀ when reacted with 0.2 ml sensitized 2.8% sheep red blood cells, as titrated above. 0.05 ml (50 µl) of this working dilution results in the same concentration (5 units of C'H₅₀) when reacted with 0.025 ml (25 µl) sensitized 2.8% sheep red blood cells, as used in the COFAL microtiter assay (Sections 4.3.7 and 4.4).

9. Determine the slope of the line joining the midpoints of the C' titration plot. First, measure from any point near the left end of the line 10 cm horizontally to the right. Then measure the vertical distance upward from the right end of the horizontal line to the slope line. Divide the vertical measurement by 10 cm to obtain the slope (1/N). The normal value for a valid slope is $0.20 \pm 10\%$.

Supplemental Assay Method for Detecting Lymphoid Leukosis Biocontamination by
the COFAL Test

ILLUSTRATION 7

Graphing Method for Complement Titration

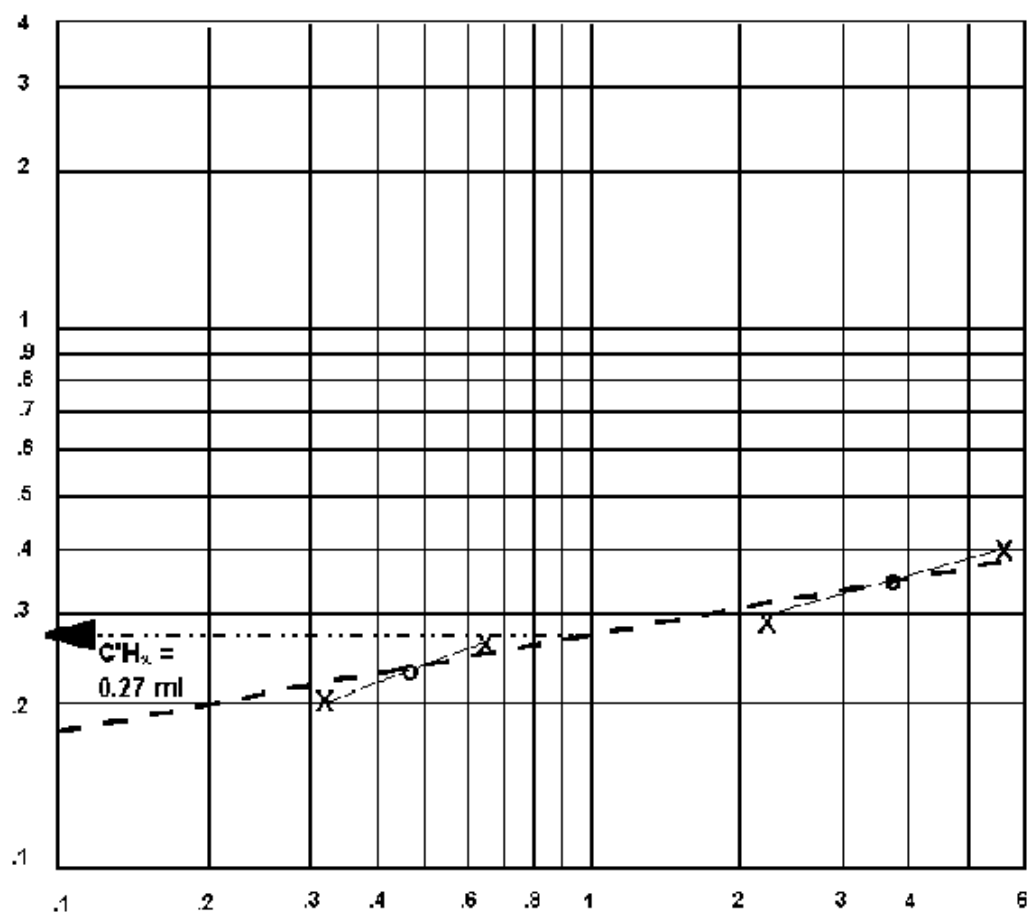

[use log-log paper]

y axis = ml volume of 1:400 dilution of C'
x axis = the ratio "% lysed/% non-lysed cells" (y/100-y)

Supplemental Assay Method for Detecting Lymphoid Leukosis Biocontamination by
the COFAL Test

ILLUSTRATION 8

Complement Dilutions for Conversion of
1 C'H₅₀ to 5 C'H_{50s} in the LBCF Test

ML C' = 1 C'H ₅₀	For 5 C'H _{50s} , Dilute Stock C'				
	1:300 C'	1:350 C'	1:400 C'	1:450 C'	1:500 C'
0.21	114	133	152	171	190
0.22	109	127	145	164	182
0.23	104	122	139	157	174
0.24	100	117	133	150	167
0.25	96	112	128	144	160
0.26	92	108	123	138	153
0.27	89	104	119	133	148
0.28	86	100	114	129	143
0.29	83	97	110	124	139
0.3	80	93	107	120	133
0.31	77	90	103	116	129
0.32	75	87	100	113	125
0.33	73	85	97	109	121
0.34	71	82	94	106	118
0.35	69	80	91	103	114

Supplemental Assay Method for Detecting Lymphoid Leukosis Biocontamination by
the COFAL Test

4.3.7 Serum and antigen titrations

The serum is a standard antiserum for the test, and the antigen is a known gs antigen-containing reagent. To conserve serum, the titrations are done in a microtiter block test system.

4.3.7.1 Preparation of serum for inactivation

1. Make an initial dilution (in 1X VBD) of positive serum which will be fourfold lower (4X) than the stated titer (if known or estimated).
2. Inactivate the diluted serum for 30 min at 56°C.
3. The diluted and inactivated antiserum may be dispensed into convenient small aliquots (sufficient for a day's test) and stored at -70°C or lower.

4.3.7.2 Addition of VBD to plates (see **Illustration 9**)

1. Add 25 μ l (0.025 ml) VBD to the wells in which the antigen dilutions are to be made, except the first one in each row. (In **Illustration 9** this includes wells 2 to 8, A through H). Also add 25 μ l to the 3 wells of the serum-complement controls (9A through 9C) and to the 5 wells of serum control (9D through 9H).
2. Add 50 μ l (0.05 ml) VBD with a pipette dropper to each of the 3 wells of the VBD complement controls (10A through 10C)
3. Add 100 μ l (0.1 ml) VBD with a pipette dropper to a well for the cell control (10H).

Anticomplementary Controls

Anticomplementary Controls												
	1	2	3	4	5	6	7	8	9	10	11	12
1.25 C'H _{50s}	A								Serum (4X) C' Control	VBD Control	X	0%
2.5 C'H _{50s}	B								Serum (4X) C' Control	VBD Control	X	10%
5.0 C'H _{50s}	C								Serum (4X) C' Control	VBD Control	X	20%
Serum dilutions	D								X/4 serum control	X	X	30%
$\frac{X}{4}$	E								X/2 serum control	X	X	40%
$\frac{X}{2}$	F								X serum control	X	100%	50%
X	G								2X serum control	X	90%	60%
2X	H								4X serum control	Red cell control	80%	70%
4X												
		1:2	1:4	1:8	1:16	1:32	1:64	1:128	1:256	Hemolysis Standards		

Antigen Dilutions

4.3.7.3 Addition of antigen to plates

1. Add 25 μ l of the test antigen to the first 2 wells of each row (1 and 2, A through H, **Illustration 9**).
2. Using a pipetter set at 25 μ l (or a 0.025 microdiluter), mix and make serial twofold dilutions starting with wells 2A through 2H and continuing to wells 8A through 8H. Discard the 25 μ l after mixing the number 8 wells.

4.3.7.4 Addition of serum to plates

1. Make serial twofold dilutions in tubes of the serum prepared in Step 1. These dilutions will be 4X (the concentration as prepared in Step 1), 2X, X (the expected titration endpoint), $\frac{X}{2}$, and $\frac{X}{4}$.
2. Add 25 μ l of the corresponding dilution of serum to the wells as shown in **Illustration 9**. The dilutions will be added to wells 1 through 9 in the appropriate row (rows D-H). The 4X concentration will also be added to wells 9A through 9C.
3. Shake the plates and allow to stand at 4°C until the complement is added. Stack or cover plates to prevent evaporation.

4.3.7.5 Preparation and addition of complement

1. Make the dilution of complement which will contain 5 C'H_{50s} in 0.4 ml (see **Section 4.3.6**). From this, make a 1:2 and a 1:4 dilution to give 2.5 and 1.25 units, respectively.
2. Add 50 μ l of this complement dilution to all wells which get 5 units of complement

(wells 1-9, rows C through H in **Illustration 9**).

3. Add 50 μ l of a 1:2 dilution of complement to all wells getting 2.5 units of C' (wells 1-9, row B).

4. Add 50 μ l of a 1:4 dilution of complement to all wells getting 1.25 units of C' (wells 1-9, row A).

5. Shake the plates and incubate at 4°-6°C for 15-18 hr. Stack or seal plates to avoid evaporation.

4.3.7.6 Addition of sensitized red cells

1. Add 25 μ l of sensitized sheep red blood cells to all the wells. Shake immediately, tape, and incubate at 37°C.

NOTE: Incubation may be done in a water jacketed incubator, or by floating the plates in a 37°C water bath for 30 min. The plates should be shaken gently every 10 min to keep the cells (remaining) in suspension or the plates may be placed on a mechanical shaker in a 37°C incubator for the 30 min period. A shaker with a reciprocal action traversing a course of 2-3 mm at approximately 250-500 times per min will keep the cells in suspension and not cause splashing. More vigorous shaking must be avoided to prevent mechanical lysis of cells or inactivation of complement.

2. After incubation, add 125 μ l (0.125 ml) of each color standard to the plates.

3. Centrifuge plates at 600 X g for 5 min or allow cells to settle at 4°C for 4-6 hr.

4. Read by comparison with color standards. Record % hemolysis on record sheets and determine optimal dilution of antigen and titer of the serum. Use 4 units of antiserum for each test.

4.4 Detection of gs antigen in test material

Store all test samples, including positive and negative controls, at -60°C or colder until the CF test is conducted. Just prior to testing, thaw and refreeze each sample (test sample and control samples) 3 times to disrupt intact cells and to release group specific antigen, if present.

The antiserum used in these tests is one produced in rabbits against the P-27 antigen of an avian leukosis virus. This reagent will be supplied by the Center for Veterinary Biologics-Laboratory.

4.4.1 Test wells

Add reagents in the following order: (See **Illustration 10**)

1. Add 25 µl VBD to all test wells, rows A-H, wells 1-9).
2. Using a pipetter set at 25 µl (or a 0.025-ml microdiluter), add appropriate antigen suspension to the first well of each test series and make the 1:2, 1:4, 1:8 dilutions. Change the pipette tips (or blot the diluter) and pick up another aliquot of antigen to make the 1:2 anti-complementary test dilution.

ILLUSTRATION 10. Template for CF plate.

	1	2	3	4	5	6	7	8	9	10	11	12
A	1:2									X	0%	Serum A/C
B	1:4									X	10%	Pos. Ag A/C
C	1:8									X	20%	5 C'H ₅₀
D	A/C 1:2									X	30%	2.5 C'H ₅₀
E	1:2									X	40%	1.25 C'H ₅₀
F	1:4									100%	50%	Red cell control
G	1:8									90%	60%	Pos. Ag Pos. Serum
H	A/C 1:2									80%	70%	X

Color Stds

3. Add 25 μ l of 4X or 4 unit antiserum to all test wells receiving antiserum (not the anti-complementary test wells). Add 25 μ l for VBD to the anti-complementary test wells.
4. Shake plates and stack to prevent evaporation until complement is added.
5. Prepare working dilution of C' as determined in **Section 4.3.6**. Add 50 μ l to all the test wells (rows A-H, wells 1-9). This is best done late in the afternoon. Shake plates and incubate at 4°C for 15-18 hr. Stack or cover to prevent evaporation.
6. Add 25 μ l of the prepared presensitized red cells to all wells. Tape and seal plates. Place on a slow speed reciprocal shaker at 37°C and agitate constantly (with just enough force to keep the cells from settling) for 30 min. Remove from incubation and centrifuge at 600 X g for 5 min.
7. Read by comparison with color standards and record % hemolysis.

4.4.2 Control wells

Only 1 set of controls is needed for each group of tests. These additions are made at the same time as the test wells.

1. In Row 12, add VBD to the following: 25 μ l to wells A and B; 50 μ l to wells C, D, and E; and 100 μ l to well F.
2. Add 25 μ l antiserum (4 units) to wells 12A and 12G.
3. Add 25 μ l of a positive antigen control (4 units) to wells 12B and 12G.

4. Add 50 µl working dilution complement to wells 12A, 12B, 12C, and 12G. Dilute complement 1:2 and add 50 µl to well 12D. Dilute complement 1:4 and add 50 µl to well 12E.

5. Add 25 µl sensitized red cells to all wells and proceed as in the screening tests. For samples of results of completed test see **Illustration 11.**

ILLUSTRATION 11. Sample plate readings.

	N-1 1	N-2 2	N-3 3	S1-1 4	S1-2 5	S1-3 6	S2-1 7	S2-2 8	S2-3 9	10	11	12	
A 1:2	100	100	100	0	0	0	100	100	100	X	0%	100	Serum A/C
B 1:4	100	100	100	30	0	0	100	100	100	X	10%	100	Pos. Ag. A/C
C 1:8	100	100	100	70	10	0	100	100	100	X	20%	100	5 C'H ₅₀
D A/C 1:2	100	100	100	100	100	100	100	100	100	X	30%	100	2.5 C'H ₅₀
E 1:2	100	30	20	0	0	0	0	0	0	X	40%	50- 70	1.25 C'H ₅₀
F 1:4	100	80	40	0	0	0	0	0	0	100%	50%	0	Red cell control
G 1:8	100	100	100	20	0	0	30	0	0	90%	60%	0	Pos. Ag. Pos. Serum
H A/C 1:2	100	100	100	100	100	100	100	100	100	80%	70%	X	
	S3-1	S3-2	S3-3	R1-1	R1-2	R1-3	R2-1	R2-2	R2-3	Color stds			

N = uninoculated culture
R = positive control culture

S = test sample culture
Number in square = % hemolysis

5. Report of test results

Presence of complement-fixing activity in the harvested samples (from passages) at the 1:4 or higher dilution, in the absence of anticomplementary activity, is considered positive unless the activity can definitely be established to be caused by something other than infectious lymphoid leukosis virus. Activity at the 1:2 dilution is considered to be suspicious, and the sample must be further subcultured to determine the presence or absence of the group-specific antigen.

5.1 Record the results as percentages for each dilution of each passage, and report the final results of each test as negative/satisfactory or positive/unsatisfactory.

5.2 Report "no test" in case of reagent or control failure and specify which.

6. Repeat tests

The decision to repeat a test will be made according to the merits of each situation.

7. References

7.1 Sarma, P. S., H. C. Turner, and R. J. Huebner. An avian leukosis group specific complement-fixation reaction. Application for the detection and assay of non-cytopathogenic leucosis viruses. Virology 23:313-321 (1964).

7.2 Public Health Monograph No. 74. Standardized diagnostic complement fixation method and adaptation of micro test (1965). U.S. Department of Health, Education and Welfare, Washington, D.C. 20201.

7.3 A Guide to the Performance of the Standardized Diagnostic Complement Fixation Method and Adaptation to Micro Test. 1st Edition, July 1, 1969. U.S. Department of Health, Education, and Welfare, Washington, D.C. 20201.

7.4 Sever, J. L. Application of a microtechnique to viral serological investigations. J. Immunol. 88:320-329 (1962).

7.5 Code of Federal Regulations, Title 9, Part 113.31 U.S. Government Printing office, Washington, D.C., 2000.

8. Summary of revisions

This document was completely revised and rewritten in new format to 1) meet the current NVSL/CVB QA requirements, 2) update the reagent and equipment lists, 3) allow for alternate methods of cell culture preparation and handling, 4) include treatment methods for additional vaccines, and 5) to provide additional testing clarification. No significant changes were made from the superseded protocol.

9. Appendix 1 - Counting Cells in Suspension with a Neubauer Hemacytometer and Formulating Cell Suspensions

The protocol in this appendix describes a method to count cells in suspension with the use of a 1/10 mm deep Neubauer hemacytometer and microscope. It also explains how to formulate cell suspensions for specific concentrations and volumes.

9.1 Materials

9.1.1 Equipment/instrumentation

Equivalent equipment or instrumentation may be substituted for any brand name listed below.

1. Hemacytometer (1/10 mm deep Neubauer hemacytometer)
2. Incandescent microscope (capable of 100X magnification)
3. Hand Tally Counter (Daigger Cat. No. GX6594)

9.1.2 Reagents/supplies

Equivalent reagents or supplies may be substituted for any brand name listed below.

1. Trypan Blue (0.4%), refer to current version of PYRPP0090
2. Snap cap tube, 6 ml, 12 X 75 mm, (Falcon, Cat. No. 2058)
3. Disposable plastic pipettes, 1, 5, 10, and 25 ml
4. Pipette (Labsystems, Model Finnpiquette Digital 5-40 μ l)
5. Disposable pipette tips

9.2 Counting cells with a hemacytometer

In a 6-ml snap cap tube, dilute 0.5 ml of the cell suspension to be counted with 1.0 ml of 0.4% Trypan Blue solution. Replace the cap on the tube and mix the suspension by inverting the tube several times. Place the cover slip over the counting grid on the hemacytometer. While the cells are still suspended, quickly load the chamber of the hemacytometer with this preparation using a pipette. Fill the chamber with enough of the preparation to completely cover the grid under the cover slip. Overfilling can cause erroneous counts. The total volume of cell suspension in 10 1-mm squares (see numbered squares) under the cover slip is equal to 1 cubic mm or 1 μ l.

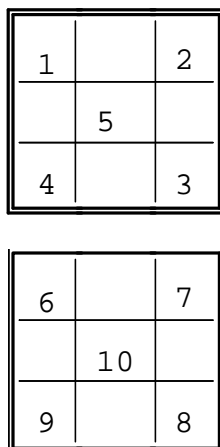


Figure 1.

Let the preparation stand for approximately 1 min to allow the cells to settle onto the bottom of the counting chamber. Examine the grid with a microscope under 100X magnification. Check for the even distribution of cells. (Any irregularity of distribution will cause erroneous results.) Count the live cells (dead cells stain blue while live cells remain translucent). Count only those live cells that fall on the top line, the left line, or within each numbered 1-mm square (1-10) in the grid (Figure 1). Keep track of the total number of cells counted for the 10 squares with a Hand Tally Counter.

Calculate the number of cells per ml in the initial suspension by multiplying the total cell count by the dilution in Trypan Blue (3) and by the conversion factor from cubic mm (μ l) to ml (1000). See example below.

```

Example:  number of cells in 10 squares=    385
           1:3 cell dilution=     x    3
                                   1155
           cubic mm/ml         x 1000
number of cells per ml= 1155000
    
```


9.3 Formulating cell suspensions

9.3.1 First calculate the Dilution Factor (DF) by dividing the concentration of cells/ml in the initial suspension by the desired final concentration of cells/ml.

Example:

If the concentration of cells in the initial suspension is 1155000 cells/ml and the desired final concentration is 350000 cells/ml, then:

$$DF = 1155000 \text{ cells/ml} \div 350000 \text{ cells/ml} = 3.3$$

9.3.2 Next, divide the desired final volume of cells by the DF. The result of this division will tell you the volume of the initial cell suspension you will need to make the final desired volume of cells.

Example:

If the final desired volume of cells is 375 ml, then:

$$375 \text{ ml} / 3.3 \text{ (DF)} = 113.6 \text{ ml}$$

This is the volume of the initial cell suspension needed to make the final volume of cells. (Round this number to 114.)

9.3.3 Finally, take the amount of the initial cell suspension determined in **Section 9.3.2** and add sufficient media to bring it to the final volume of cells desired.

Example:

Add 261 ml (375 ml - 114 ml) of media to 114 ml of the initial cell suspension (1155000 cells/ml) to get 375 ml of the desired 350000 cells/ml suspension.